

## DAkKS Calibration

of Torque Sensors  
and Torque Measurement Chains  
according to Calibration Standards  
DIN 51309, EURAMET/cg-14,  
DAkKS-DKD-R 3-5



D-K-17603-01-00

Torque Measuring Range  
1 N·m - 200 N·m  
Uncertainty of Measurement 1·10<sup>-4</sup>

## Proprietary Calibration

of Torque Sensors  
Force Sensors  
and Measuring Chains

## QM-System



Our Quality Management Systems acc. to  
DIN EN ISO 9001:2015 and  
DIN EN ISO/IEC 17025 for Laboratories

## Accreditation



The Accreditation of our Calibration  
Laboratory was conducted by the DAkKS  
(Deutsche Akkreditierungsstelle)

- Automotive Industry
- Automation Technology
- Production Technology
- Development and Research Institutes
- Aerospace
- Machine Building
- Chemical Industry
- Food Industry
- Medical Technology
- Universities
- Academies

You  
have a  
**Measuring Task**






we  
have the  
**Solution**



Lorenz Messtechnik GmbH  
Obere Schloßstraße 131  
D-73553 Alfdorf  
Tel. +49 (7172) 93730-0  
Fax. +49 (7172) 93730-22  
Internet : [www.lorenz-sensors.com](http://www.lorenz-sensors.com)  
E-Mail: [info@lorenz-sensors.com](mailto:info@lorenz-sensors.com)  
Internet: [www.lorenz-messtechnik.de](http://www.lorenz-messtechnik.de)  
E-Mail: [info@lorenz-messtechnik.de](mailto:info@lorenz-messtechnik.de)






# Torque Sensors

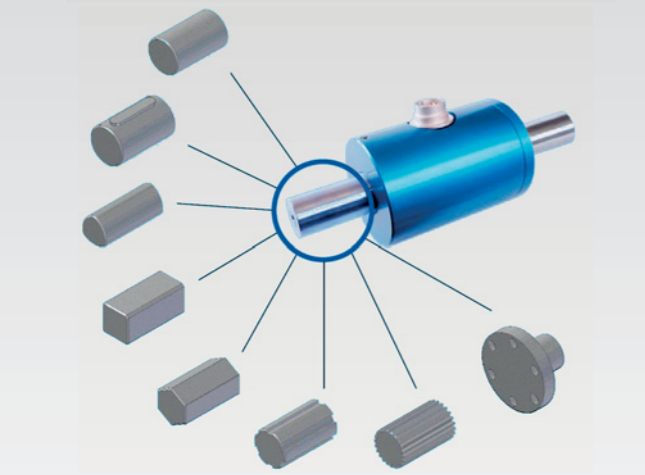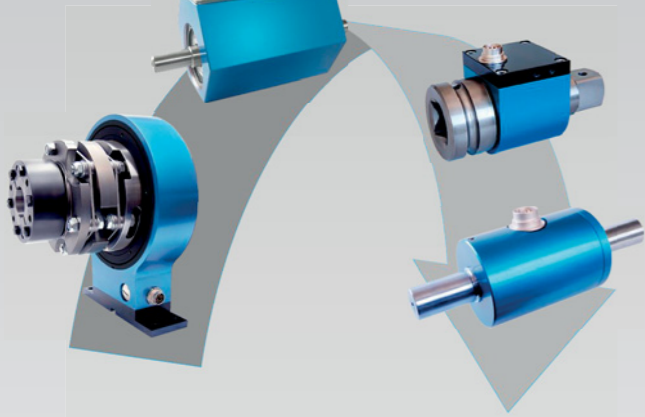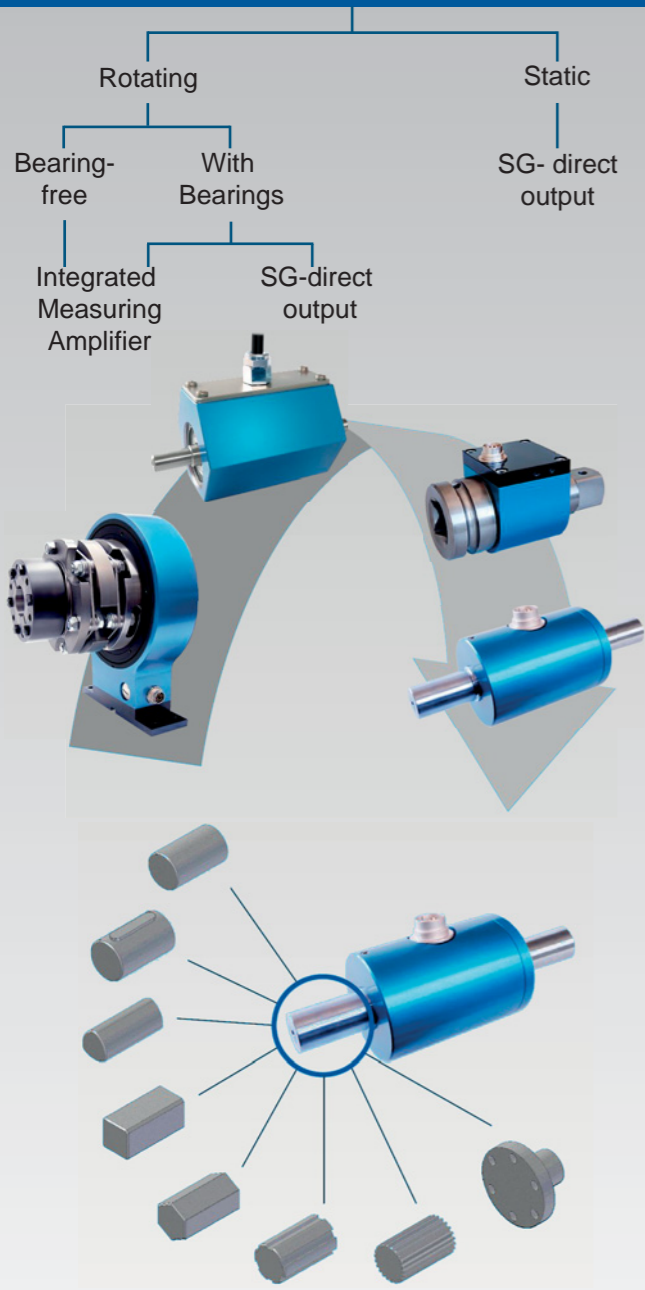

0.005 N·m ... 20 kN·m  
from class 0.05

# Force

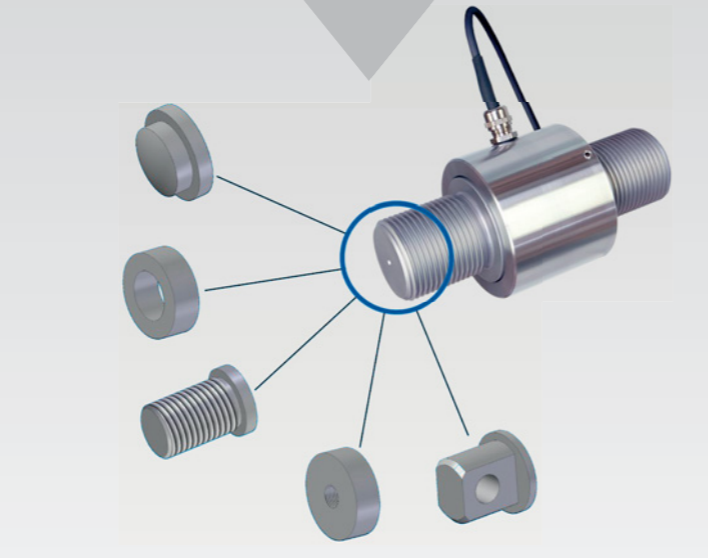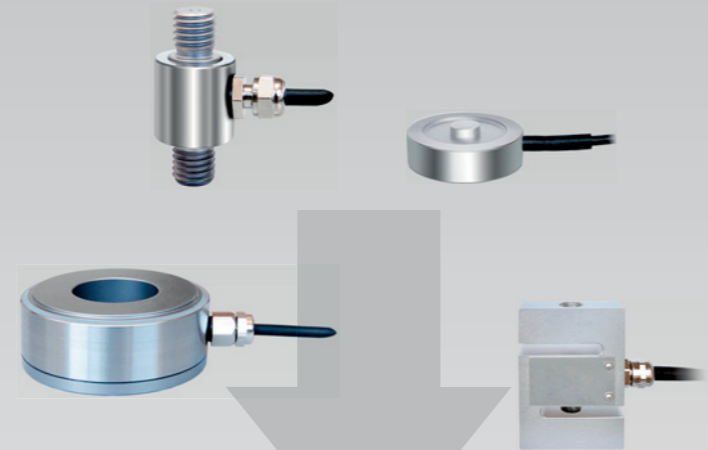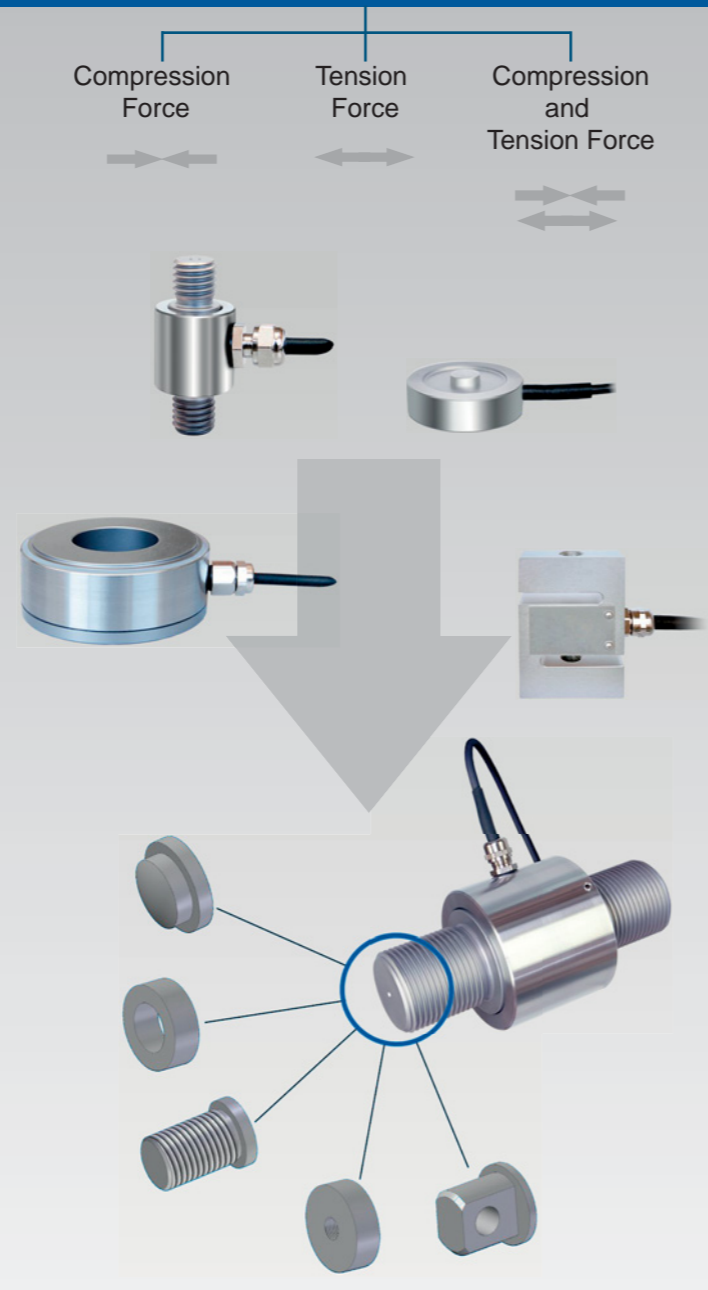

10 N ... 5 MN  
from class 0.05

# Measuring Amplifiers

- Sensor-Interfaces
- Portable
- Table and Laboratory
- Assembly




## Connection Possibilities

- |                 |                  |
|-----------------|------------------|
| Undefined scale | e.g. mV/V; mA    |
| Defined scale   | e.g. N; N·m      |
| PC-connection   | e.g. USB; serial |

# Test Benches

- Torque-Testing Devices
- Motor Test Benches
- Force Test Benches
- Testing Devices for Windshield Wiper Rods

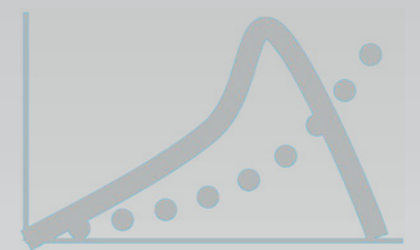

Torque Calibration System for Bottom Bracket Bearings



Motor Test Bench